Dr. Maisch

Any Column, Any Size, Any Media

ReproSil pHoenix

Extreme pH-stable

MADE BY DR. MAISCH

CONTENT

- p 4 - WHY IS THERE A NEED TO DO CHROMATOGRAPHY AT EXTREME pH?
- p 5 - EFFECT OF EXTREME pH ON SILICA BASED MEDIA
  - INCREASING pH STABILITY
- p 6 - 7 - LONG TERM pH STABILITY
- p 8 - SELECTIVITY COMPARISON BASIC CONDITIONS pH 12
- p 9 - SELECTIVITY COMPARISON AT DIFFERENT pH
- p 10 - 11 - SELECTIVITY AND PEAK SHAPE UNDER BASIC AND ACIDIC ELUENT CONDITIONS

ReproSil pHoenix
MADE BY DR. MAISCH

From one of the biggest **H**igh-**P**erformance **L**iquid **C**hromatography (HPLC) - Column Manufacturer in Europe.

Ako nás možno kontaktovať:

AZ CHROM s.r.o.
Robotnícka 10
831 03 Bratislava
Tel. 0907 244526
azetchrom@hplc.sk
www.azetchrom.sk

WHY IS THERE A NEED TO DO CHROMATOGRAPHY AT EXTREME pH?

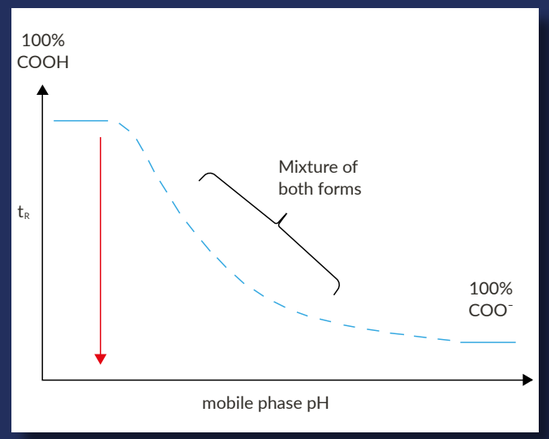

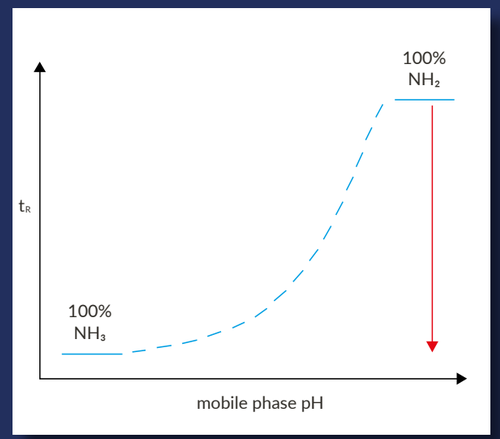

$RCOOH \leftrightharpoons RCOO^- + H^+$

Acids are best retained with optimal peak shape at low pH

$RNH_2 \leftrightharpoons RNH_3^+ + OH^-$

Bases are best retained with optimal peak shape at high pH

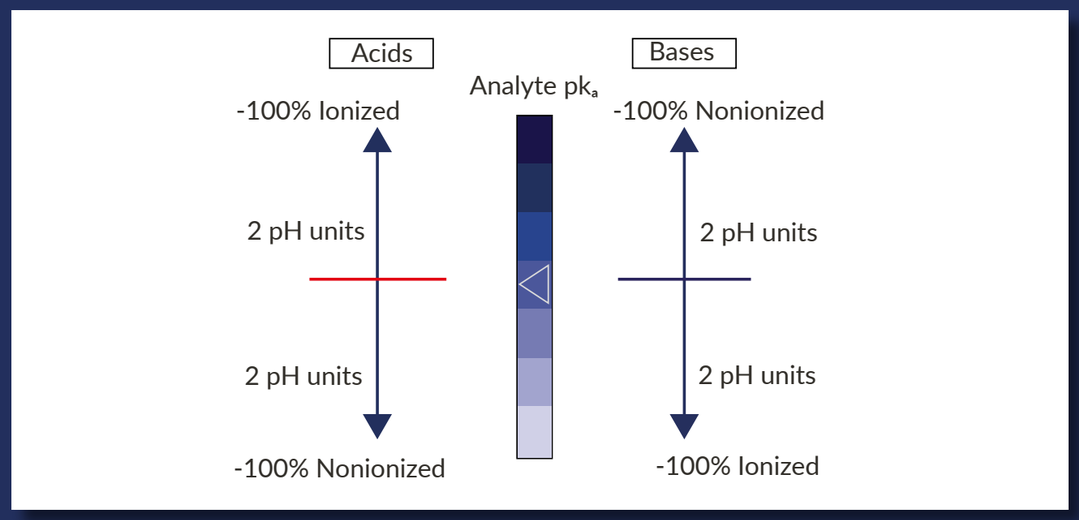

EFFECT OF EXTREME pH ON SILICA BASED MEDIA

High pH:

Hydrolysis of silica gel backbone

→ Severe peak distortion
→ loss of efficiency

Low pH:

Hydrolysis of bonded phase and endcapping

→ Loss of retention time
→ Peak tailing for basic compounds

INCREASING pH STABILITY

NEW HYBRID DOUBLE SHIELDED SILICA

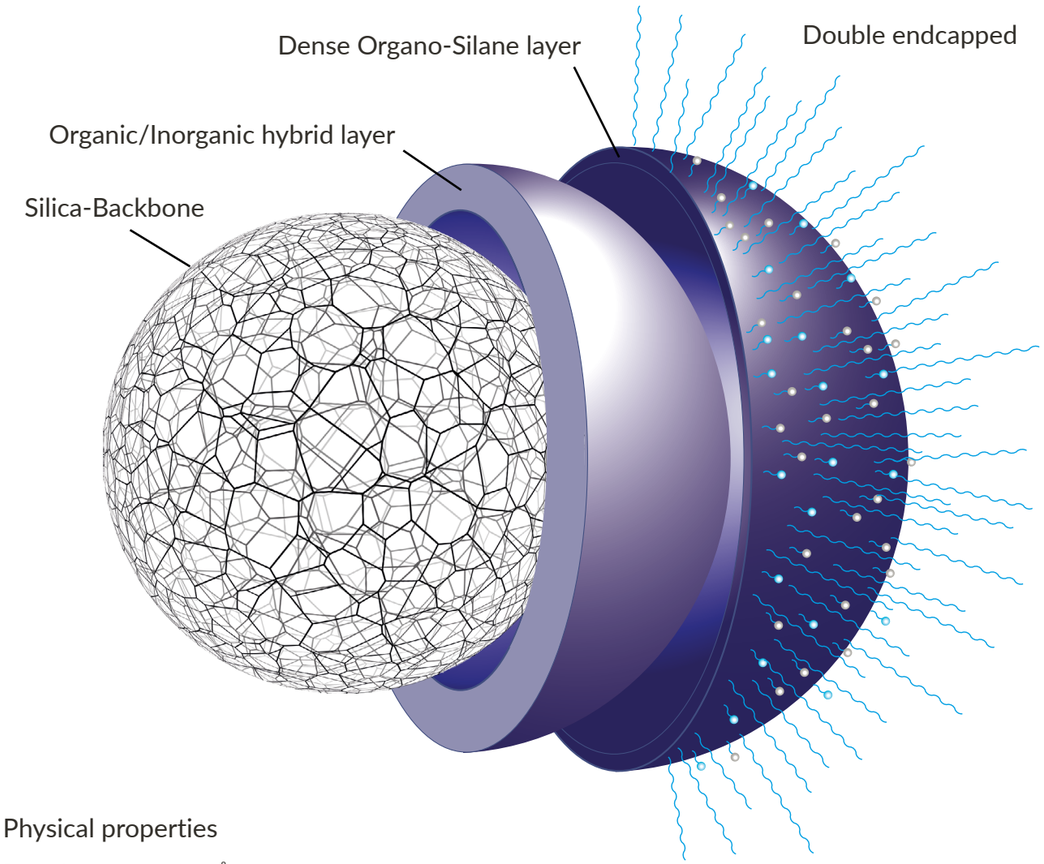

Physical properties

Pore size:	100 Å
Particle size:	1.9 µm, 3 µm, 5 µm, 7 µm, 10 µm
Surface area:	470 m²/g
Modification:	C18
Carbon content:	22%
Endcapping:	yes

www.dr-maisch.com

Purging conditions:
NaOH(aq) pH 12

Test conditions:

Mobile phase: MeOH/H_2O 85/15
Flow rate: 1 ml/min
Detector: UV @ 254 nm

Name:	Conc. mg / mL
1 Uracil	0.015
2 Phenol	0.700
3 N,N-Diethyl-M-Toluamide	0.600
4 Toluene	4.000

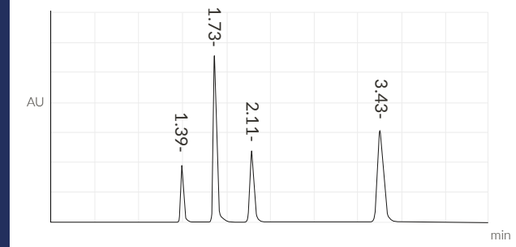

0 hours

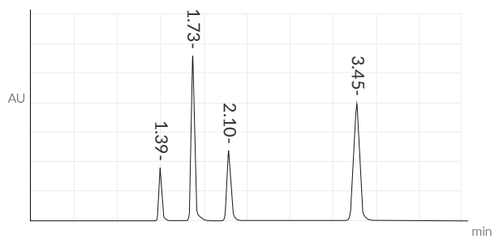

210 hours

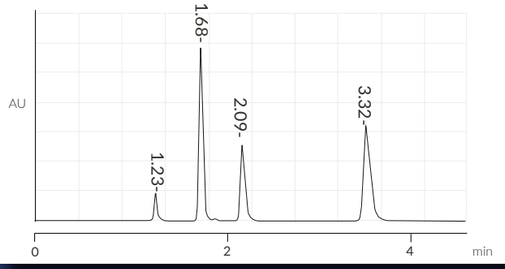

400 hours

LONG TERM pH STABILITY

Peak retention vs. purging time with NaOH(aq) pH 12

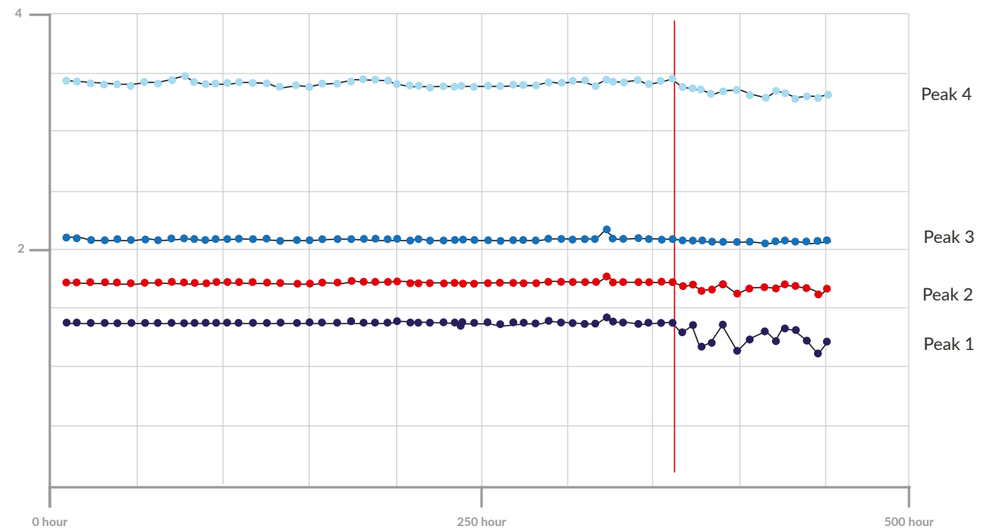

Th. plates (Peak 4) % vs. purging time

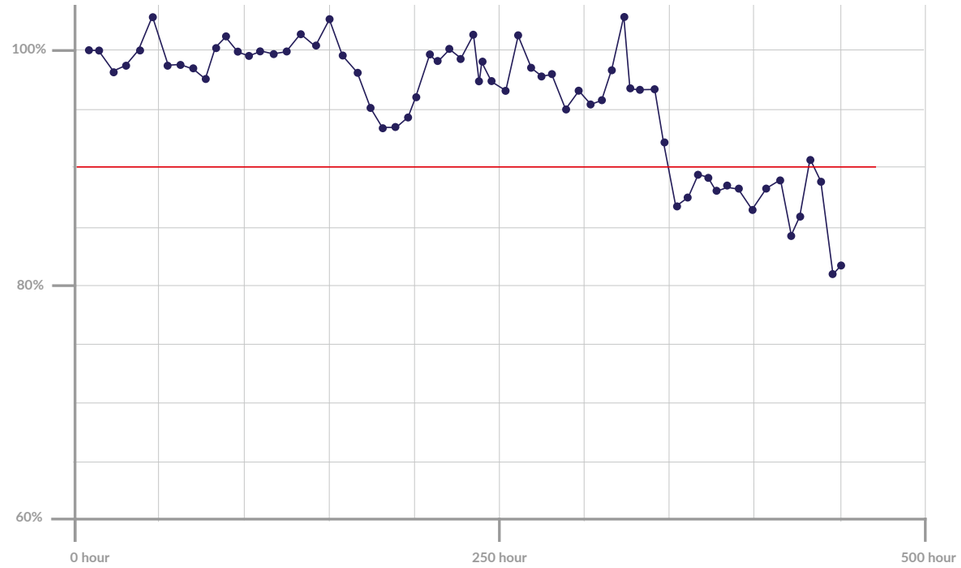

Resolution of „impurity“ on ReproSil pHoenix

Mobile phase: MeOH/NH_3-resolution (pH 12) 85/15
Flow rate: 1 ml/min
Detector: UV @ 254 nm

Name:	Conc. mg / mL
1 Uracil	0.015
2 Phenol	0.700
3 N,N-Diethyl-M-Toluamide	0.600
4 Toluene	4.000

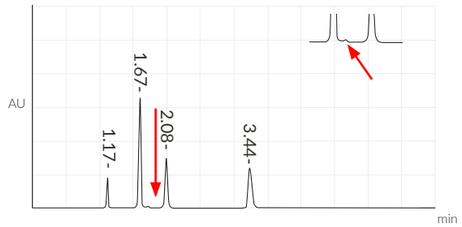

ReproSil pHoenix

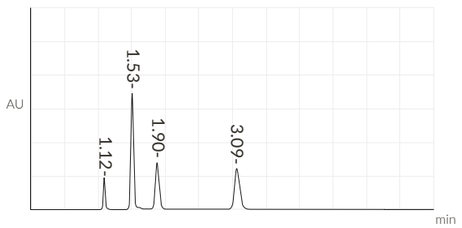

Kromasil Eternity

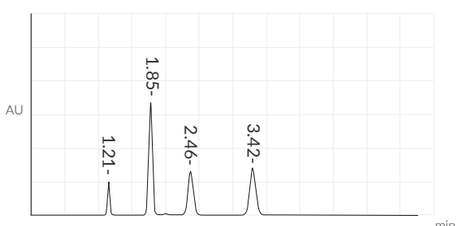

YMC Triart

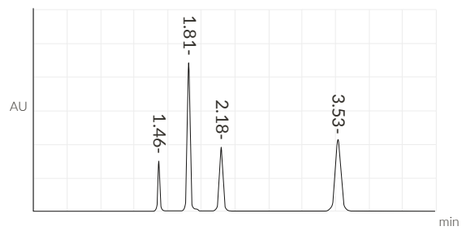

ReproSil pHoenix, pH 7

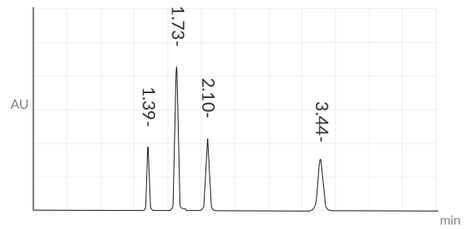

ReproSil pHoenix, pH 3

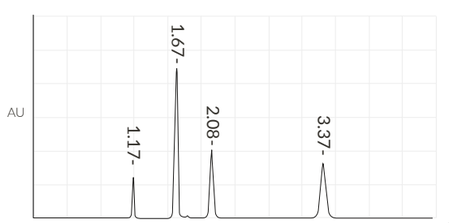

ReproSil pHoenix, pH 12

SELECTIVITY AND PEAK SHAPE UNDER BASIC AND ACIDIC ELUENT CONDITIONS

Observe superior selectivity / resolution of ReproSil pHoenix vs. Waters Acquity

Data courtesy of Nuvisan ICB GmbH

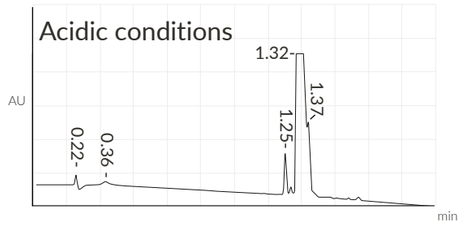

Waters Acquity

Column: Acquity UPLC BEH C18 1.7 µm, 50x2.1mm;
eluent A: water + 0.1 vol% formic acid;
eluent B: acetonitrile;
gradient: 0-1.6 min 1-99 % B, 1.6-2.0 min 99 % B

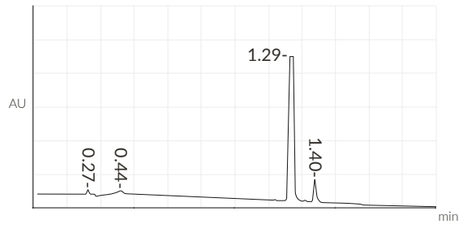

ReproSil pHoenix

Column: ReproSil pHoenix C18 3 µm, 75 x 2.1 mm;
eluent A: water + 0.1 vol% formic acid;
eluent B: acetonitrile;
gradient: 0-1.6 min 1-99 % B, 1.4-2.0 min 99 % B

Observe superior peak shape of ReproSil pHoenix vs. Waters Acquity

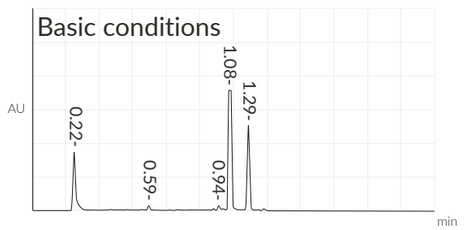

Waters Acquity

Column: Acquity UPLC BEH C18 1.7 µm, 50x2.1mm;
eluent A: water + 0.2 vol% aqueous ammonia (32%);
eluent B: acetonitrile;
gradient: 0-1.6 min 1-99 % B, 1.6-2.0 min 99 % B

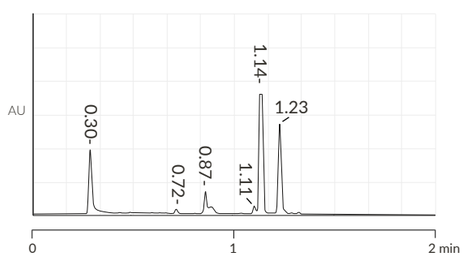

ReproSil pHoenix

Column: ReproSil pHoenix C18 3 µm, 75 x 2.1 mm;
eluent A: water + 0.2 vol% aqueous ammonia (32%);
eluent B: acetonitrile;
gradient: 0-1.4 min 1-99 % B,1.4-2.0 min 99 % B

SELECTIVITY AND PEAK SHAPE UNDER BASIC AND ACIDIC ELUENT CONDITIONS

Observe superior selectivity / resolution and peak shape of ReproSil pHoenix vs. Waters Acquity

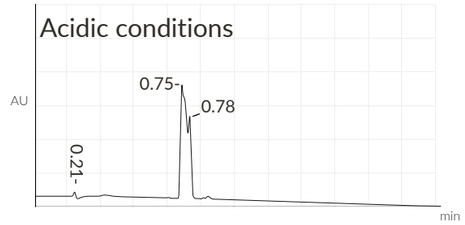

Waters Acquity

Column: Acquity UPLC BEH C18 1.7 µm, 50x2.1mm;
eluent A: water + 0.1 vol% formic acid;
eluent B: acetonitrile;
gradient: 0-1.6 min 1-99 % B, 1.6-2.0 min99 % B

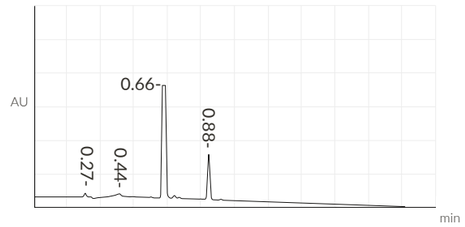

ReproSil pHoenix

Column: ReproSil pHoenix C18 3 µm, 75 x 2.1 mm;
eluent A: water + 0.1 vol% formic acid;
eluent B: acetonitrile;
gradient: 0-1.6 min 1-99% B, 1.4-2.0 min99% B

Observe superior peak shape of ReproSil pHoenix vs. Waters Acquity

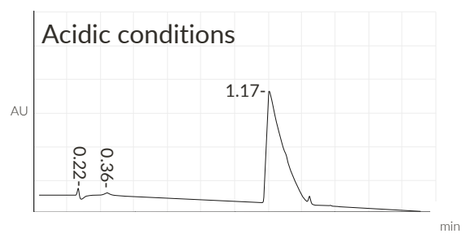

Waters Acquity

Column: Acquity UPLC BEH C18 1.7 µm,50x2.1mm;
eluent A: water + 0.1 vol% formic acid;
eluent B: acetonitrile;
gradient: 0-1.6 min 1-99 % B, 1.6-2.0 min 99 % B

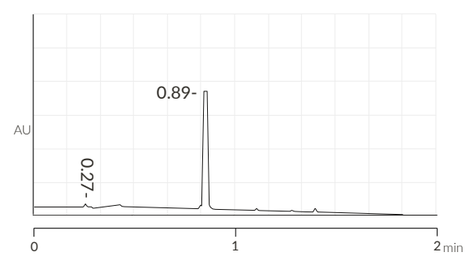

ReproSil pHoenix

Column: ReproSil pHoenix C18 3 µm, 75 x 2.1 mm;
eluent A: water + 0.1 vol% formic acid;
eluent B: acetonitrile;
gradient: 0-1.6 min 1-99 % B, 1.4-2.0 min 99 % B

www.dr-maisch.com

Dr. Maisch

Any Column, Any Size, Any Media

Ako nás možno kontaktovať:

AZ Chrom s.r.o.
Robotnícka 10
831 03 Bratislava
Tel. 0907 244526
azetchrom@hplc.sk
www.azetchrom.sk

pHoenix

Dr. Maisch HPLC GmbH
Beim Brückle 14
D-72119 Ammerbuch
T: +49 7073 50357
F: +49 7073 4216
www.dr-maisch.com
www.modcol.com
E-Mail: info@dr-maisch.com

PDF brochure
for download